

GDS-3000A Series

650/350MHz Digital Storage Oscilloscope

FEATURES

- 650/350MHz Bandwidth, 2 Input Channels
- 5GSa/s Real-time Sampling Rate (One Channel);
2.5GSa/s Real-time Sampling Rate (Dual Channels)
- Per Channel 200Mpts Memory Depth
- 200,000 wfm/s of Waveform Update Rate
- 10.2 inch 800*480 TFT LCD Display
- 490,000 Segments of Segmented Memory and the Waveform Search Function to Optimize the Efficiency of Record Length
- Zoom Window and Play/Pause Rapidly Navigate the Waveforms
- 38 sets of Automatic Measurement Offer Various Measurement Selections
- High Resolution Acquisition Mode
- I²C/UART/CAN/LIN Serial Bus Trigger and Decoding Functions
- Dual Channel Spectrum Analyzer (DC~2.5GHz) with spectrogram
- Dual Channel 25MHz Arbitrary Waveform Generator
- Optional 13 Sets of Power Analysis Measurements
- Optional 16 Digital Channels with a Logic Analyzer(MSO)
- Flexible Remote Control Connectivity (Standard: USB/LAN/RS-232; Option: GPIB)

GWINSTEK
Simply Reliable

One Oscilloscope with Time Domain, Frequency Domain and Power Measurement.



GDS-3000A digital storage oscilloscopes have 650MHz and 350MHz models with two-channel and 16-channel logic analyzer options.

The series features the memory length of each channel up to 200Mpts; the sampling rate of 5GSa/s one channel and 2.5GSa/s on dual channels. Its display is 10.2" TFT LCD and it provides the color display mode.

Accurate Signal Acquisition and Analysis

GDS-3000A strengthens many functions and specifications required for oscilloscope measurements including the memory depth of up to 200Mpts per channel. The advantage of long memory is that it allows users to maintain high sampling rate even at low speed time settings; the waveform update rate is up to 200,000wfms; and the segmented memory can capture and analyze up to 490,000 segments.

For measurement, GDS-3000A incorporates the Fine scale function to allow users to fine-tune the vertical scale according to the requirements so as to achieve full scale measurement to improve its measurement accuracy. With a 10.2" large screen display and the acquisition method with the high resolution mode allow low-noise signals under high-bandwidth measurements. In addition, the series is equipped with 1M ohm and 50 ohm input impedance selections, which can be set according to different DUT measurement requirements to achieve the effect of impedance matching. The search function can quickly find the signals that meet the conditions according to the needs of the test. The cursor mark function allows users to clearly observe the voltage (or current), time and delta data of each point measured by the cursor. Via the indicator function, the measured range is to be shown at the specific section of the waveform.

Dual Domain Measurement

For frequency domain measurement, it is equipped with a dual channel spectrum analyzer, which allows users to measure and analyze the frequency domain signals of two channels at the same time. It is also equipped with Spectrogram function, which allows users to easily observe complex frequency domain fluctuations that are proportionally decomposed into simple superimposed waves so as to understand the signal strength distribution. The soft keys allow users to have more intuitive settings for operation, which can improve the measurement efficiency.

13 Sets of Switching Mode Power Supply Measurements

GDS-3000A provides a rich measurement items for switch mode power supply testing. The provided power supply test items include AC input analysis items: Power Quality, Harmonics, Inrush Current; DC output analysis required test items: Ripple/Noise, Transient Response Analysis, Turn On/OFF, Efficiency; Control Loop response(Bode) and PSRR(Power Supply Rejection Ratio); Complete switching component analysis items: Modulation, Switching loss, SOA(Safe Operation Area) and Magnetics analysis: B-H curve. On one side of GDS-3000A, a power supply for 50MHz (GCP-530) and 100MHz(GCP-1030) current probes is provided. This feature can save users the cost of purchasing the power supply for current probes and relief the burden of carrying the power supply when going out.


GDS-3000A is standardly equipped with a dual-channel 25MHz arbitrary waveform generator and the frequency response analysis function. The FRA has the load function, which can load multiple FRA measurement results for comparison. User define shortcut key provides user-definable shortcut keys. The use of the shortcut key can improve measurement efficiency.

GDS-3000A provides a rich communication interfaces. In addition to the commonly used USB Host, USB Device port, and LAN port, it also includes a highly stable RS232 interface and an optional GPIB interface.

SELECTION GUIDE


Model	GDS-3352A	GDS-3652A
Bandwidth	350MHz	650MHz
Channels	2	2
Record Length	200M / CH	200M / CH
Real-time Sampling Rate	Max. 5 GSa/s	Max. 5 GSa/s
Built-in	Dual Channel Spectrum Analyzer(DC~2.5GHz) with Spectrogram	

A. 10.2 INCH, 8 BITS RGB COLOR GRADIENT DISPLAY

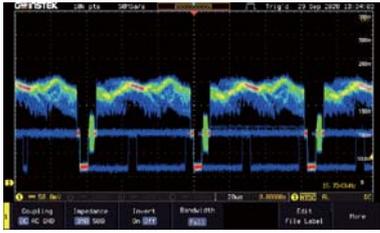

With respect to the waveform display technology, the GDS-3000A series oscilloscope is capable of displaying RGB color gradients with 8 bits each which can delineate the profound gradational fluctuations; as if it can recreate the analog oscilloscope display capability. When a composite signal is input, the GDS-3000A series, has the ability to precisely reveal the colored burst signal and to show details of layers with the brightness. Hence, the dull monochrome waveform is imbued with vitality, it allows users to easily determine and analyze waveforms.

B. 200M MEMORY DEPTH PER CHANNEL INDEPENDENTLY

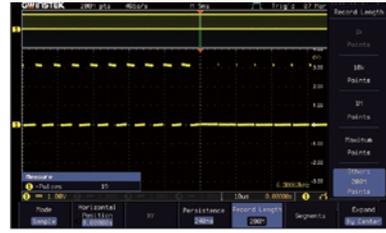

The GDS-3000A series oscilloscope has a powerful and incomparable memory depth for the data retrieving. 200M memory depth per channel independently surpasses the specification of the industry's 3000 series DSO boundary. 200M memory depth allows users to easily seize the waveform detail while conducting fundamental measurement applications.

C. FINE SCALE



The Fine scale function is incorporated to allow users to fine-tune the vertical scale according to their needs to achieve full-scale measurement and improve the accuracy of the voltage or current measurements.

D. HIGH RESOLUTION ACQUISITION MODE



The acquisition method with high resolution mode is provided to effectively remove noise and improve the accuracy of automatic measurement.

E. 38 ITEMS OF AUTO MEASUREMENT SELECTION AND THE STATISTICS FUNCTION






The GDS-3000A series soundly provides 38 measurement items. Based upon the parameters such as voltage, current, time, frequency, and delay measurement, users can decide which measurement items to choose. On the single display screen, the GDS-3000A series provides 8 measurement selections.

The statistics mode can also be selected for users to analyze the mean value, the maximum, the minimum, and standard deviation of the retrieved waveforms to ensure signal's integrity and identify abnormal waveforms.

Users can also use the Measure Shortcuts function to select the item to be measured, and then store the selected item in Shortcut 1~4, which can be selected to conduct measurements for the same product next time. Users just select the previously stored Shortcut 1~4 without making new selections from Add measurement, and all the measurement items will be displayed on the screen to improve the measurement efficiency.

F. 490,000 SEGMENTED MEMORY

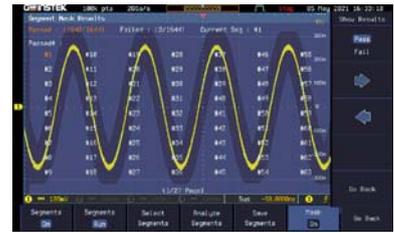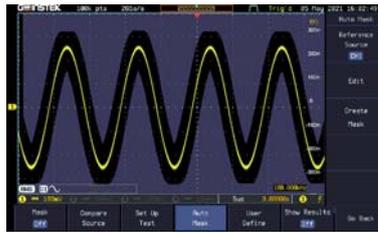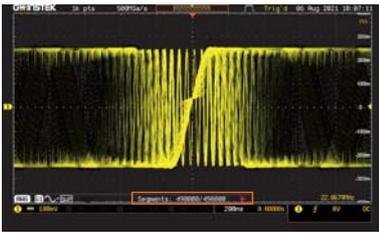


In addition, GDS-3000A incorporates the Mask determination function under Segment, allowing users to quickly analyze abnormal waveforms that exceed the target range.

As the length of the sampling memory increases to 200Mpts, the number of acquisitions that can be set in the GDS-3000A's segmented memory at one time has also increased significantly, and up to 490,000 waveforms can be stored continuously (under the condition of the memory length of 1,000pts).

The segmented memory allows users to capture and observe interesting waveforms. Through the statistical function, it is especially helpful for finding sporadic problems in continuous events.


G. WAVEFORM SEARCH FUNCTION



Users can rapidly search desired waveforms according to the trigger condition. After activating the search function, hollow inverted triangles will show the location met the trigger condition. The upper left hand corner Overall will show the total number of waveforms met the trigger condition. Users can set waveform search by the trigger condition such as Edge, pulse width, Runt, Rise/Fall, and Bus.

When the trigger condition is met, hollow inverted triangles will appear. Users can save all marks to compare with the next input signal. The front panel of the GDS-3000A Series controls waveform zoom-out and play/pause function to swiftly identify each desired event. The function allows users to conveniently complete waveform search and save marks for rapid comparison and analysis.


H. USER DEFINE KEY

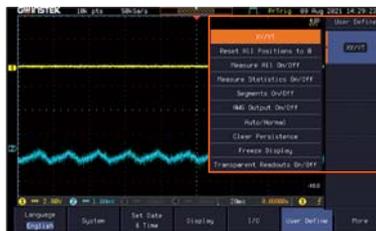


GDS-3000A incorporates a User Define key to allow users to set any one of the ten functions of User Define based upon the measurement requirement, including XY/YT; Reset all positions to 0; Measure all On/Off; Measure statistics On/Off; Segments On/Off; AWG output On/Off; Auto/Normal; Clear persistence; Freeze display and transparent readouts On/Off.

Users can quickly select the function setting by just pressing a key to quickly meet the measurement needs so as to improve the measurement efficiency.


I. SPECTRUM ANALYZER FUNCTION

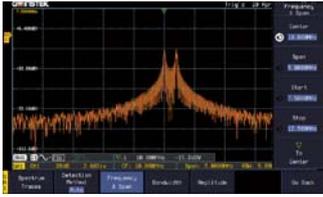


Spectrum Analyzer

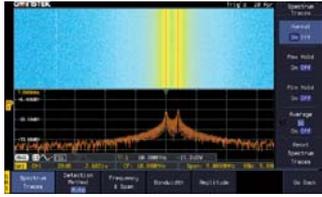

Spectrum Analyzer + Spectrogram

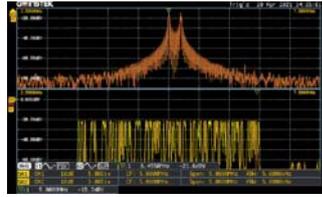

Dual Spectrum Analyzer

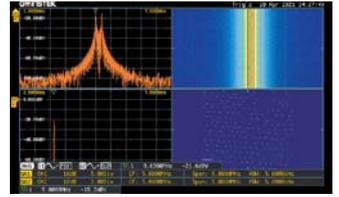


Dual Spectrum Analyzer + Spectrogram

For frequency domain measurement, dual channel spectrum analyzer is equipped. Users can measure and analyze dual channel frequency domain signals at the same time. It also includes the Spectrogram function, which allows users to easily observe the signal's strength distribution and the relationship of the spectrum distribution over time. The independent numeric key input on the panel makes the operation more convenient for users, thereby improving the measurement efficiency. For promotion selling point, dual Spectrum Analyzer and Spectrogram can test the frequency response of the left and right channels of the Audio Amplifier at the same time.

The above displays are :

1. Spectrum Analyzer
2. Spectrum Analyzer + Spectrogram
3. Dual Spectrum Analyzer
(Dual channels can set different conditions)
4. Dual Spectrum Analyzer + Spectrogram

J. 25MHZ DUAL CHANNEL ARBITRARY WAVEFORM GENERATOR

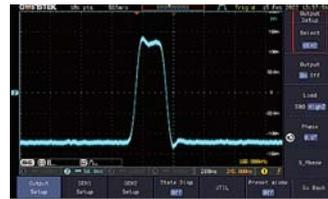


* The above two displays are load from CH1, and then it was generated by AWG to CH2

GDS-3000A is standardly equipped with a 25MHz dual channel arbitrary waveform generator, and provides built-in Sine, Square, Pulse, Ramp, DC, Noise, Sinc, Gaston, Lorentz, Exponential Rise, Exponential Fall, Haversine, Cardiac and other waveforms. Users can be directly input the amplitude and frequency of the signal through the numeric keys. Compared with the previous model, the new function is that users can select the arbitrary waveform

function of the AWG to store the signal measured by the analog channel of the oscilloscope to the arbitrary waveform of the signal source (UAW file), or it can directly output this signal from the signal generator, which is a new function that allows users to conveniently generate various measured signals to simulate diversified signal outputs.

K. PC REMOTE CONTROL (WEB SERVER FUNCTION)

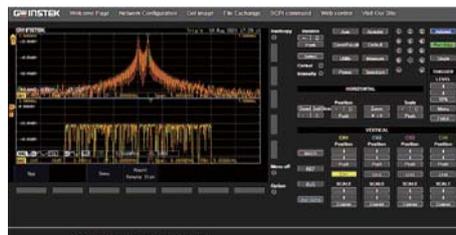

GDS-3000A has a built-in Web Server function to allow users to connect GDS-3000A's Web Server by using a browser in the same network domain via Ethernet connection. System information can be obtained and the oscilloscope screen (.png file) can be observed and captured remotely.

GDS-3000A can be controlled remotely through GUI to download and upload configuration files and test SCPI commands. Users can use this function to obtain oscilloscope information and configuration files, and operate remote control even if they are not on-site.

L. POWER ANALYSIS FUNCTIONS



13 Sets of Switching Mode Power Supply Measurements

In daily life, switching power supplies have become the mainstream of power supplies. Engineers often have to rack their brains in order to improve product performance and reduce switching loss, and Ripple/Noise.


GDS-3000A has an option of rich measurement items for switching mode power supply testing. To meet engineers' measurement needs for switching mode power supply, rich measurement function can help engineers save a lot of measurement computing time and improve product development efficiency.



Power Quality

For AC voltage and current measurement, its distortion and other abnormal phenomena will affect the power consumption, efficiency and reliability of the power supply.

Measurement items: current/voltage root mean square value, actual power, reactive power, frequency, power factor, phase angle, +/- V Peak, +/- I Peak, AC/DC voltage and current, voltage/current crest factor, impedance, resistance and reactance.

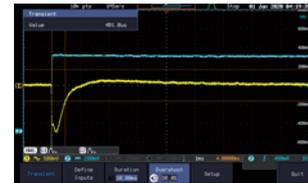

Transient Response Analysis

Output analysis required test items: Ripple/Noise, Transient response analysis, Turn On/OFF and Efficiency. It measures the time required for the output DC voltage to reach the stable level expected by users when the output load changes suddenly.

Measurement item: transient response value (s).




Switching Loss

Switching component analysis items: Switching loss, SOA (Safe Operation Area) and Modulation analysis. Analyze the integral of the product of the voltage and current of the switching device (MOSFET or IGBT) in the power supply, and then measure the switching loss of the device, including Turn-on switching loss, Turn-off switching loss and Conduction loss. The higher the switching frequency, the higher the Turn-on and Turn-off switching loss. Measurement items: power loss, energy loss & $R_{ds(on)}/V_{ce(sat)}$.



Control Loop Response

Control Loop Response and PSRR (Power Supply Rejection Ratio) PSRR: Power supply rejection ratio (PSRR) analysis, which is used to confirm that power equipment suppresses ripple noise in different frequency ranges. Measurement items: frequency and PSRR (dB).

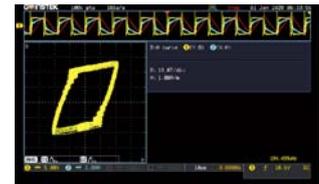

Magnetics Analysis

Magnetics Analysis(B-H Curve): The characteristics of magnetic materials are divided into magnetic flux density (B), magnetic field strength (H) and material magnetic permeability (μ). The B-H diagram is usually used to verify the saturation of the magnetic components in the switch power supply. Measurement items: Measure the voltage and current flowing through the magnetic component and draw a B-H diagram.

M. OPTIONAL 16-CHANNEL LOGIC ANALYZER



GDS-3000A can be upgraded to a mixed-signal oscilloscope (MSO) by selecting an optional 16-channel logic analyzer, which is a plugin. When you have several GDS-3000As, you can plug in an optional logic analyzer to other unit at any time without installing any software.

Users can analyze digital signals, I²C, UART, CAN, LIN and parallel bus through a logic analyzer.

PANEL INTRODUCTION



- | | | |
|---|---|---|
| 1. Hardcopy Key | 8. Math, Reference & Bus Keys | 15. VGA Ooutput |
| 2. Function Keys | 9. User Define Key | 16. RS232 Interface |
| 3. Number Keys | 10. Logic Analyzer and Arbitrary Waveform Generator Functions | 17. USB Device Port |
| 4. Power Analysis and Spectrum Analyzer Functions | 11. Logic Analyzer Probe Connector | 18. LAN Port |
| 5. Trigger Controls | 12. Trigger Out/Calibration Output | 19. GPIB Interface (Optional; Factory Install) |
| 6. Zooming Controls | 13. Go/NoGo Output | 20. Power Supply Output for GCP-530 or GCP-1030 Current Probe |
| 7. Search Function | 14. Dual Channel Arbitrary Function Generator Output | |

SPECIFICATIONS

		GDS-3352A	GDS-3652A
VERTICAL	Channels	2Ch+EXT	
	Bandwidth	DC~350MHz(-3dB)@50Ω/1MΩ input impedance	DC~650MHz(-3dB)@50Ω input impedance; DC~500MHz(-3dB)@1MΩ input impedance
TRIGGER	Calculated Rise Time	1ns	535ps
	Bandwidth Limit	20M/100M/200MHz ⁻¹	20M/100M/200M/300MHz ⁻¹
	Vertical Resolution	8 bits (Max.12bits with Hi Res)	*1. The tolerance of bandwidth limit is±10%.
	Vertical Resolution(1MΩ)	1mV ² ~ 10V/div	*2. The bandwidth is limited to 20MHz at 1mV/div and 2mV/div.
	Vertical Resolution(50Ω)	1mV ² ~ 1V/div	
	Input Coupling	AC, DC, GND	
	Input Impedance	1MΩ// 22pF approx.	
	DC Gain Accuracy	1mV : ±5% full scale ; ≥2mV : ±3% full scale	
	Polarity	Normal , Invert	
	Maximum Input Voltage(1MΩ)	300Vrms, CAT II	
Maximum Input Voltage(50Ω)	5 Vrms		
Offset Position Range	For 1MΩ input impedance:1mV/div~20mV/div;±1V;50mV/div~500mV/div;±10V;1V/div~5V/div;±100V;10V/div;±1000V		
Waveform Signal Process	For 50Ω input impedance:1mV/div~50mV/div;±1V;100mV/div~1V/div;±10V +, -, X, Y, FFT, User Defined Expression FFT; Spectral magnitude. Set FFT Vertical Scale to Linear RMS or dBV RMS, and FFT Window to Rectangular, Hamming, Hanning or Blackman.		
EXT TRIGGER	Source	CH1, CH2, Line , EXT	
	Trigger Mode	Auto(Supports Roll Mode for 100ms/div and slower), Normal, Single	
HORIZONTAL	Trigger Type	Edge, Pulse Width(Glitch), Video, Pulse Runt, Rise & Fall(Slope),Time out, Alternate, Event-Delay(1~65,535 events),Time-Delay(Duration, 4ns~10s),Bus(I ² C,SPI,UART,CAN,LIN)	
	Trigger Holdoff Range	4ns~10s	
X-Y MODE	Coupling	AC, DC, LF rej. , Hf rej. , Noise rej.	
	Sensitivity	1div	
SIGNAL ACQUISITION	Range	±20V	
	Sensitivity	DC ~ 100MHz Approx. 100mV ; 100MHz ~ 350MHz Approx. 150mV	
CURSORS AND MEASUREMENT	Input Impedance	1MΩ±3% ~ 22pF	
	Range	1ns/div ~ 1000s/div (1-2-5 increments); ROLL : 100ms/div ~ 1000s/div	
CONTROL PANEL FUNCTION	Pre-trigger	10 div maximum	
	Post-trigger	10,000,000 div max (depend on time base)	
POWER MEASUREMENTS (Option)	Accuracy	±5ppm, about ±2ppm increase in error per year	
	Phase Shift	Channel 1, Channel 2 ±3° at 100kHz	
CURSORS AND MEASUREMENT	Real Time Sample Rate	5GSa/s one channel; 2.5GSa/s on dual channels	
	Record Length	Max.200M pts/CH	
CONTROL PANEL FUNCTION	Acquisition Mode	Normal, Average, Peak detect, High resolution, Single ; Average: Selectable from 2 ~ 256, Peak detect: 400ps	
	Number of Segments	1 ~ 490,000 maximum	
CURSORS AND MEASUREMENT	Cursors	Amplitude, Time, Gating available;Unit:Seconds(s),Hz(1/s),Phase(degree),Ratio(%)	
	Automatic Measurement	38 sets with indicator: Pk-Pk, Max, Min, Amplitude, High, Low, Mean, Cycle Mean, RMS, Cycle RMS, Area, Cycle Area, ROVShoot, FOVShoot, RPREShoot, FPREShoot, Frequency, Period, RiseTime, FallTime, +Width, -Width, Duty Cycle, +Pulses, -Pulses, +Edges, -Edges, %Flicker, Flicker ldx ,FRR, FRF, FFR, FFF, LRR, LRF, LFR, LFF, Phase.	
CONTROL PANEL FUNCTION	Cursors Measurement	Voltage difference between cursors (ΔV) Time difference between cursors (ΔT)	
	Auto Counter	6 digits, range from 2Hz minimum to the rated bandwidth	
CONTROL PANEL FUNCTION	Autoset	Single-button, automatic setup of all channels for vertical, horizontal and trigger systems, with "Undo Autoset", "Fit Screen"/ "AC Priority" mode, and "Fine Scale" functions.	
	Save Setup	20 sets	
POWER MEASUREMENTS (Option)	Save Waveform	20 sets	
	Save Reference Waveform	4 sets	
POWER MEASUREMENTS (Option)	Power Quality, Harmonics, Ripple, In-rush current, Switching Loss, Modulation, SOA, Transient, Efficiency, B-H curve, Control Loop Response, PSRR, Turn On/Off		

SPECIFICATIONS

		GDS-3352A	GDS-3652A
AWG	Channels Sample Rate Vertical Resolution Max. Frequency Waveforms Output Range Output Resolution Output Accuracy Offset Range Offset Resolution Sine Square/Pulse Ramp	2 200 Msa/s 14 bits 25 MHz Sine, Square, Pulse, Ramp, DC, Noise, Sinc, Gaston, Lorentz, Exponential Rise, Exponential Fall, Haversine, Cardiac 20 mVpp to 5 Vpp, HighZ; 10 mVpp to 2.5 Vpp, 50Ω 1mV 2% (1 kHz) ±2.5 V, HighZ; ±1.25 V, 50Ω 1mV Frequency Range: 100mHz~25MHz; Flatness (relative to 1kHz): ±0.5 dB<15MHz, ±1dB(15MHz~25MHz); Harmonic Distortion: <40 dBc; Stray (Non-harmonic): <40 dBc; Total Harmonic Distortion: 1%; S/N Ratio: 40 dB Frequency Range: 100mHz~15MHz; Rise/Fall time: <15ns; Overshoot: <3%; Duty cycle Square: 50% & Pulse: 0.4%~99.6%; Min. Pulse Width: 30 ns; Jitter: 500 ps Frequency Range: 100mHz~1MHz; Linearity: 1%; Symmetry: 0~100%	
SPECTRUM ANALYZER	Frequency Range Span Resolution Bandwidth Reference Level Vertical Units Vertical Position Vertical Scale Display Average Noise Level Spurious Response Frequency Domain Trace Types Detection Methods FFT Windows	DC ~ 2.5GHz (Max.) dual channel with spectrogram (based on advanced FFT). Notice: Frequency which exceeds analog front end bandwidth is uncalibrated 1kHz ~ 2.5GHz (Max.) 1Hz ~ 2.5MHz (Max.) -80 dBm to +40dBm in steps of 5dBm dBV RMS; Linear RMS; dBm -12divs to +12divs 1dB/div to 20dB/div in a 1-2-5 Sequence 1V/div < -40dBm, Avg: 16; 100mV/div < -60dBm, Avg: 16; 10mV/div < -80dBm, Avg: 16 2nd harmonic distortion < 35dBc; 3rd harmonic distortion < 40dBc Normal; Max Hold; Min Hold; Average (2 ~ 256) Sample; +Peak; -Peak; Average FFT Factor: Hanning 1.44; Rectangular 0.89; Hamming 1.30; Blackman 1.68	
LOGIC ANALYZER (Option)	Sample Rate Bandwidth Record Length Input Channels Trigger Type Thresholds Quad Threshold Selections User-defined Threshold Range Maximum Input Voltage Minimum Voltage Swing Vertical Resolution	Per Channel 1GSa/s 200MHz Per Channel 10M pts (max) 16 Digital (D15 - D0) Edge, Pattern, Pulse Width, Serial bus (I ² C, SPI, UART, CAN, LIN), Parallel Bus D0-D3, D4-D7, D8-D11, D12-D15 Thresholds TTL, CMOS (5V, 3.3V, 2.5V), ECL, PECL, 0V, User Defined ±5V ±40 V ±250 mV 1 bit	
FREQUENCY RESPONSE ANALYSIS	Frequency Range Input and Output Sources Number of Test Points Dynamic Range Test Amplitude Test Results Manual Measurements Plot Scaling	20 Hz ~ 25 MHz Channel 1 ~ 2 10, 15, 30, 45, 90 points per decade selectable for logarithm scale; 2 ~ 1000 points selectable for linear scale > 80 dB (typical) 10mVpp to 2.5Vpp into 50Ω, 20mVpp to 5Vpp into High-Z, Fixed test amplitude or custom amplitude for each decade. Logarithmic or linear overlaid gain and phase plot, may also overlay with reference plots for cross comparison. Test results saved in csv format for offline analysis Tracking gain and phase markers Auto-scaled during test	
DISPLAY SYSTEM	TFT LCD Type Waveform Update Rate Display Resolution Interpolation Waveform Display Display Graticule Display Mode	10.2" TFT LCD WVGA color display 200,000 wfms/sec max. 800 horizontal x 480 vertical pixels (WVGA) Sin(x)/x Dots, Vectors, Variable persistence (16ms~4s), Infinite persistence, gray and color waveforms 8 x 10 divisions YT, XY	
INTERFACE	RS-232C USB Port Ethernet Port VGA Video Port Optional GPIB Module Go/NoGo BNC Kensington Style Lock Power Supply Receptacles	DB-9 male connector USB 2.0 high-speed host port x 1; USB high-speed 2.0 device port x 1 RJ-45 connector, 10/100Mbps with HP Auto-MDIX DB-15 female connector, monitor output for display on VGA monitor Fully programmable with IEEE488.2 compliance 5V Max/10mA open collector output Rear-panel security slot connects to standard Kensington-style lock ±12V/500mA for current probe usage. 2 sets	
MISCELLANEOUS	Operating Line Voltage Range Multi-Language Menu On-Line Help Time Clock Internal Flash Disk Installed APP User Define Key	0°C ~ 50°C, Relative Humidity ≤ 80% at 40°C or below; ≤ 45% at 41°C~50°C AC 100V ~ 240V, 50Hz ~ 60Hz, auto selection. power consumption: 100W Available Available Time and date, provide the date/time for saved data 800M bytes Single-Level Cell flash memory Go/NoGo, DVM, DataLog, Digital Filter, Frequency Response Analyzer, Mask, Mount Remote Disk, Demo User can select one of the several different preset functions as shortcut key	
DIMENSIONS & WEIGHT	420(W) X 253(H) X 113.8(D)mm, Approx. 4.6 kg		

Note : Three-year warranty, excluding probes & LCD display panel.

Specifications subject to change without notice.

DS-3000AGD1BH

ORDERING INFORMATION

GDS-3652A 650MHz, 2-Channel, Digital Storage Oscilloscope

GDS-3352A 350MHz, 2-Channel, Digital Storage Oscilloscope

ACCESSORIES

User manual CD x 1, Power cord x 1

GTP-351R: 350MHz 10:1 passive probe for GDS-3352A (one per channel)

GTP-501R: 500MHz 10:1 passive probe for GDS-3652A (one per channel)

FREE DOWNLOAD

PC Software OpenWave software **Driver** LabView driver

OPTION

DS3A-PWR Power Analysis Software **DS3A-GPIB** GPIB Interface **DS3A-16LA** 16 Channel Logic Analyzer

OPTIONAL ACCESSORIES

GTP-033A 35MHz 1:1 Passive probe	GTL-248 GPIB Cable, Double Shielded, 2000mm
GTP-352R 350MHz 20:1 Passive probe	GTL-110 Test lead, BNC to BNC connector
GDP-025 25MHz High voltage differential probe	GTL-232 RS-232C cable, 9-pin female to 9-pin female, Null modem for computer
GDP-050 50MHz High voltage differential probe	
GDP-100 100MHz High voltage differential probe	
GCP-300 300kHz/200A Current probe	GTL-246 USB 2.0 cable, A-B type cable 4P, 1800mm
GCP-500 500kHz/150A Current probe	
GCP-530 50MHz/30A Current probe	GRA-443-E Rack Adapter Panel
GCP-1000 1MHz/70A Current probe	GKT-100 Deskew Fixture
GCP-1030 100MHz/30A Current probe	

GOOD WILL INSTRUMENT CO., LTD.

No.7-1, Jhongsing Road, Tucheng Dist., New Taipei City 236, Taiwan

T +886-2-2268-0389 F +886-2-2268-0639

E-mail: marketing@goodwill.com.tw



Website



Facebook



LinkedIn

GW INSTEK

Simply Reliable